


File: C:\MassLynx\DEFAULT.PRO\ACQUDB\default.ipr

Instrument: ACQ-TQD#QBB1665

Printed: Tuesday, September 27, 2022 14:03:20 W. Europe Daylight Time

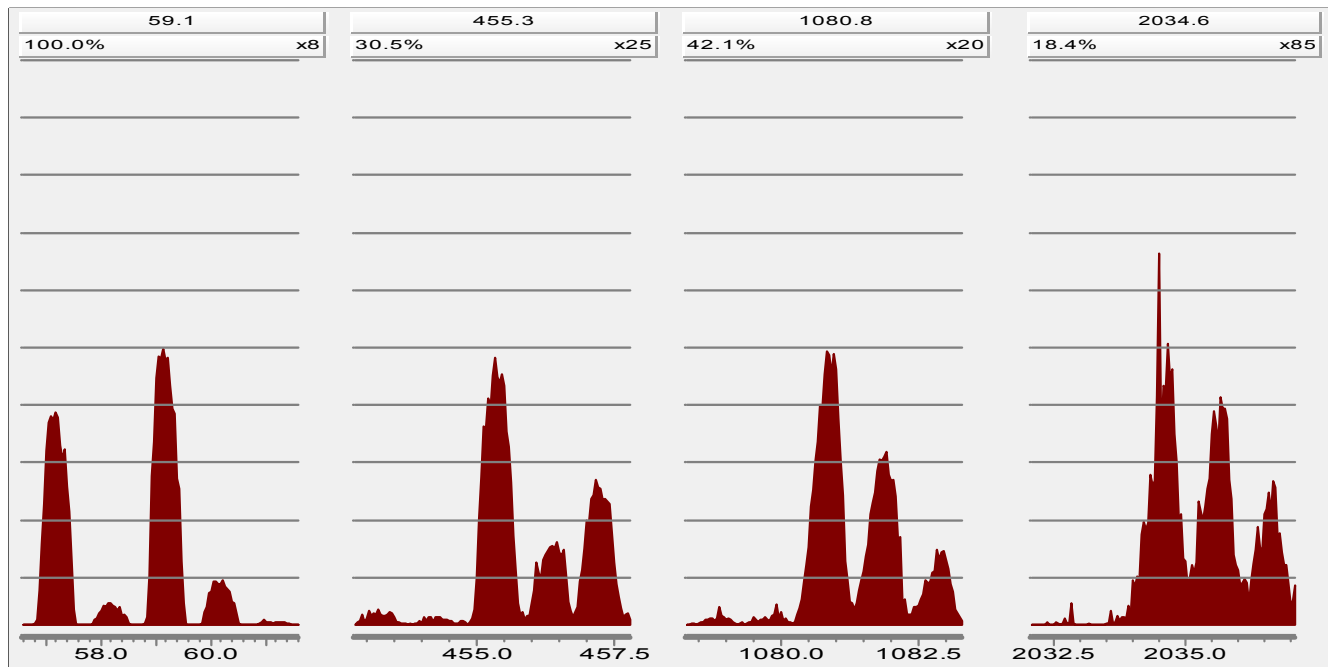

Type	Start Mass	End Mass	Set Mass
MS Scan	56.60	61.60	
MS Scan	452.80	457.80	
MS Scan	1078.30	1083.30	
MS Scan	2032.10	2037.10	

Source (ES+)	Settings	Readbacks
Capillary (kV)	3.00	2.99
Cone (V)	48.00	47.13
Extractor (V)	4.00	1.22
RF (V)	0.20	
Source Temperature (°C)	90	89
Desolvation Temperature (°C)	200	198
Cone Gas Flow (L/Hr)	0	1
Desolvation Gas Flow (L/Hr)	650	644
Collision Gas Flow (mL/Min)	0.30	0.00

Analyser	Settings	Readbacks
LM 1 Resolution	15.00	
HM 1 Resolution	15.00	
Ion Energy 1	0.40	
MS Mode Entrance	50.00	
MS Mode Collision Energy	2.00	
MS Mode Exit	50.00	
MSMS Mode Entrance	1.00	
MSMS Mode Collision Energy	31.00	
MSMS Mode Exit	1.00	
LM 2 Resolution	15.00	
HM 2 Resolution	15.00	
Ion Energy 2	3.00	
Gain	1.00	
Multiplier	-497.99	
Active Reservoir	B	

Pressure Gauges	Settings
Collision Cell Pressure (mbar)	7.082356e-004

File: C:\MassLynx\DEFAULT.PRO\ACQUDB\default.ipr  
Instrument: ACQ-TQD#QBB1665  
Printed: Tuesday, September 27, 2022 14:03:20 W. Europe Daylight Time

---

**Instrument Configuration**

Automatic Mode

MS 1 Delay Table:

	R	delay
<= 0.500	0.005	
<= 2.000	0.008	
<= 4.000	0.010	
<= 11.000	0.012	
> 11.000	0.014	

MS 2 Delay Table:

	R	delay
<= 8.000	0.005	
<= 25.000	0.006	
> 25.000	0.007	

**Engineer**

MS1 Low Mass Position	520
MS1 High Mass Position	170
MS1 Low Mass Resolution	513
MS1 High Mass Resolution	1667
MS1 Resolution Linearity	867
MS1 High Mass DC Balance	-0
MS1 DC Polarity	Negative
MS2 Low Mass Position	519
MS2 High Mass Position	192
MS2 Low Mass Resolution	513
MS2 High Mass Resolution	1686
MS2 Resolution Linearity	858
MS2 High Mass DC Balance	0
MS2 DC Polarity	Negative
HM RF Lens Correction +	0
HM RF Lens Correction -	0