

G1316A

Thermostat Test

Passed

DE43645708
A.06.04[001]
TCC

Evaluates the cooling and heating performance of the two peltier elements.


**Started at 9/17/2025 10:03:43 AM by dell-PC\dell on DELL-PC using Agilent Lab Advisor
- Version B.02.09 [195] - Basic**

Results

Item	Value	Result
Cool rate of right heat exchanger	4.0 °C/min	
<i>Minimum cooling rate</i>	2 °C/min	Passed
Heat rate of right heat exchanger	8.3 °C/min	
<i>Minimum heating rate</i>	3 °C/min	Passed
Cool rate of left heat exchanger	4.0 °C/min	
<i>Minimum cooling rate</i>	2 °C/min	Passed
Heat rate of left heat exchanger	8.4 °C/min	
<i>Minimum heating rate</i>	3 °C/min	Passed

Finished at 9/17/2025 10:11:05 AM

Signals

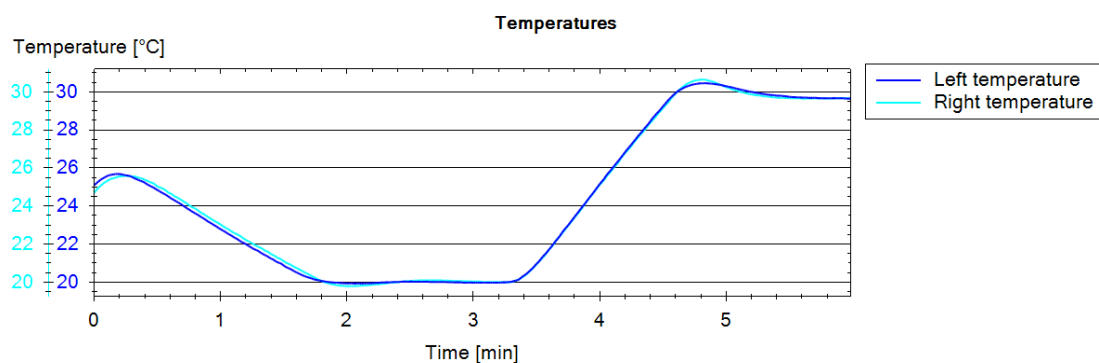

Signature: